

# T3<sup>®</sup> and Osseotite<sup>®</sup> Parallel Walled Implant Surgical Kit Reusable Drill Usage Chart

## PSKT

Use a dry erase marker to track the total number of osteotomy preparations that are performed with each drill. It is recommended that reusable drills be replaced after 15 uses. \*Single use drills should be disposed of after each procedure.



IMPLANT	ACTPSD	ACT2010	ACT2015	ACT2020	PD100	ACT2710	ACT2715	ACT2720	ACT3010	ACT3015	ACT3020	ACT3110	ACT3115	ACT3120	ACT3210	ACT3215	ACT3220	ICD100	CD500	ACT3810	ACT3815	ACT3820	ACT4285	ACT4213	ACT4218	CD600	ACT4885	ACT4813	ACT4818	ACT5285	ACT5213	ACT5218						
	ACT <sup>®</sup> Pointed Starter Drill	ACT Twist Drill 2 mm x 10 mm	ACT Twist Drill 2 mm x 15 mm	ACT Twist Drill 2 mm x 20 mm	Pilot Drill 2/3 mm	ACT Twist Drill 2.75 mm x 10 mm	ACT Twist Drill 2.75 mm x 15 mm	ACT Twist Drill 2.75 mm x 20 mm	ACT Twist Drill 3 mm x 10 mm	ACT Twist Drill 3 mm x 15 mm	ACT Twist Drill 3 mm x 20 mm	ACT Twist Drill 3.15 mm x 10 mm	ACT Twist Drill 3.15 mm x 15 mm	ACT Twist Drill 3.15 mm x 20 mm	ACT Twist Drill 3.25 mm x 10 mm	ACT Twist Drill 3.25 mm x 15 mm	ACT Twist Drill 3.25 mm x 20 mm	C'sink Drill 4 mm	C'sink Drill 5 mm	ACT Twist Drill 3.85 mm x 10 mm	ACT Twist Drill 3.85 mm x 15 mm	ACT Twist Drill 3.85 mm x 20 mm	ACT Twist Drill 4.25 mm x 8.5 mm	ACT Twist Drill 4.25 mm x 13 mm	ACT Twist Drill 4.25 mm x 18 mm	C'sink Drill 6 mm	ACT Twist Drill 4.85 mm x 8.5 mm	ACT Twist Drill 4.85 mm x 13 mm	ACT Twist Drill 4.85 mm x 18 mm	ACT Twist Drill 5.25 mm x 8.5 mm	ACT Twist Drill 5.25 mm x 13 mm	ACT Twist Drill 5.25 mm x 18 mm						
6.0	✓	A	B	C	✓										A	B	C		✓	A	B	C	A	B	C	✓	A	B	C									
5, 5/4	✓	A	B	C	✓										A	B	C		✓	A	B	C																
4, 4/3	✓	A	B	C	✓				A	B	C							✓																				
3.25	✓	A	B	C	✓	A	B	C																														
Time To Order New Drills	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1				
	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2			
	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3	3		
	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4	4		
	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5	5		
	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6	
	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	7	
	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8	8
	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9	9
	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10
	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11	11
	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12	12
	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13	13
	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14
	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	15	

\*Single use drills must be disposed of after each procedure. This chart is intended to be used as a reference guide only. The number of uses per drill will vary and depends on a variety of factors including bone density encountered, proper handling and cleaning. Refer to Instructions for Use (IFU) for Biomet 3i Kits and Instruments (P-ZBDINSTRP) available at ifu.biomet3i.com for complete Cleaning and Sterilization Information.


NOTE: Surgical instruments are susceptible to damage for a variety of reasons including but not limited to: prolonged use, misuse, rough or improper handling, inadequate cleaning, etc. Care must be taken to avoid compromising the intended performance of the instrument.

# KNOW HOW TO IDENTIFY EXCESSIVE WEAR

Dull Cutting Edge

Rounded Tip

Rounded Corner

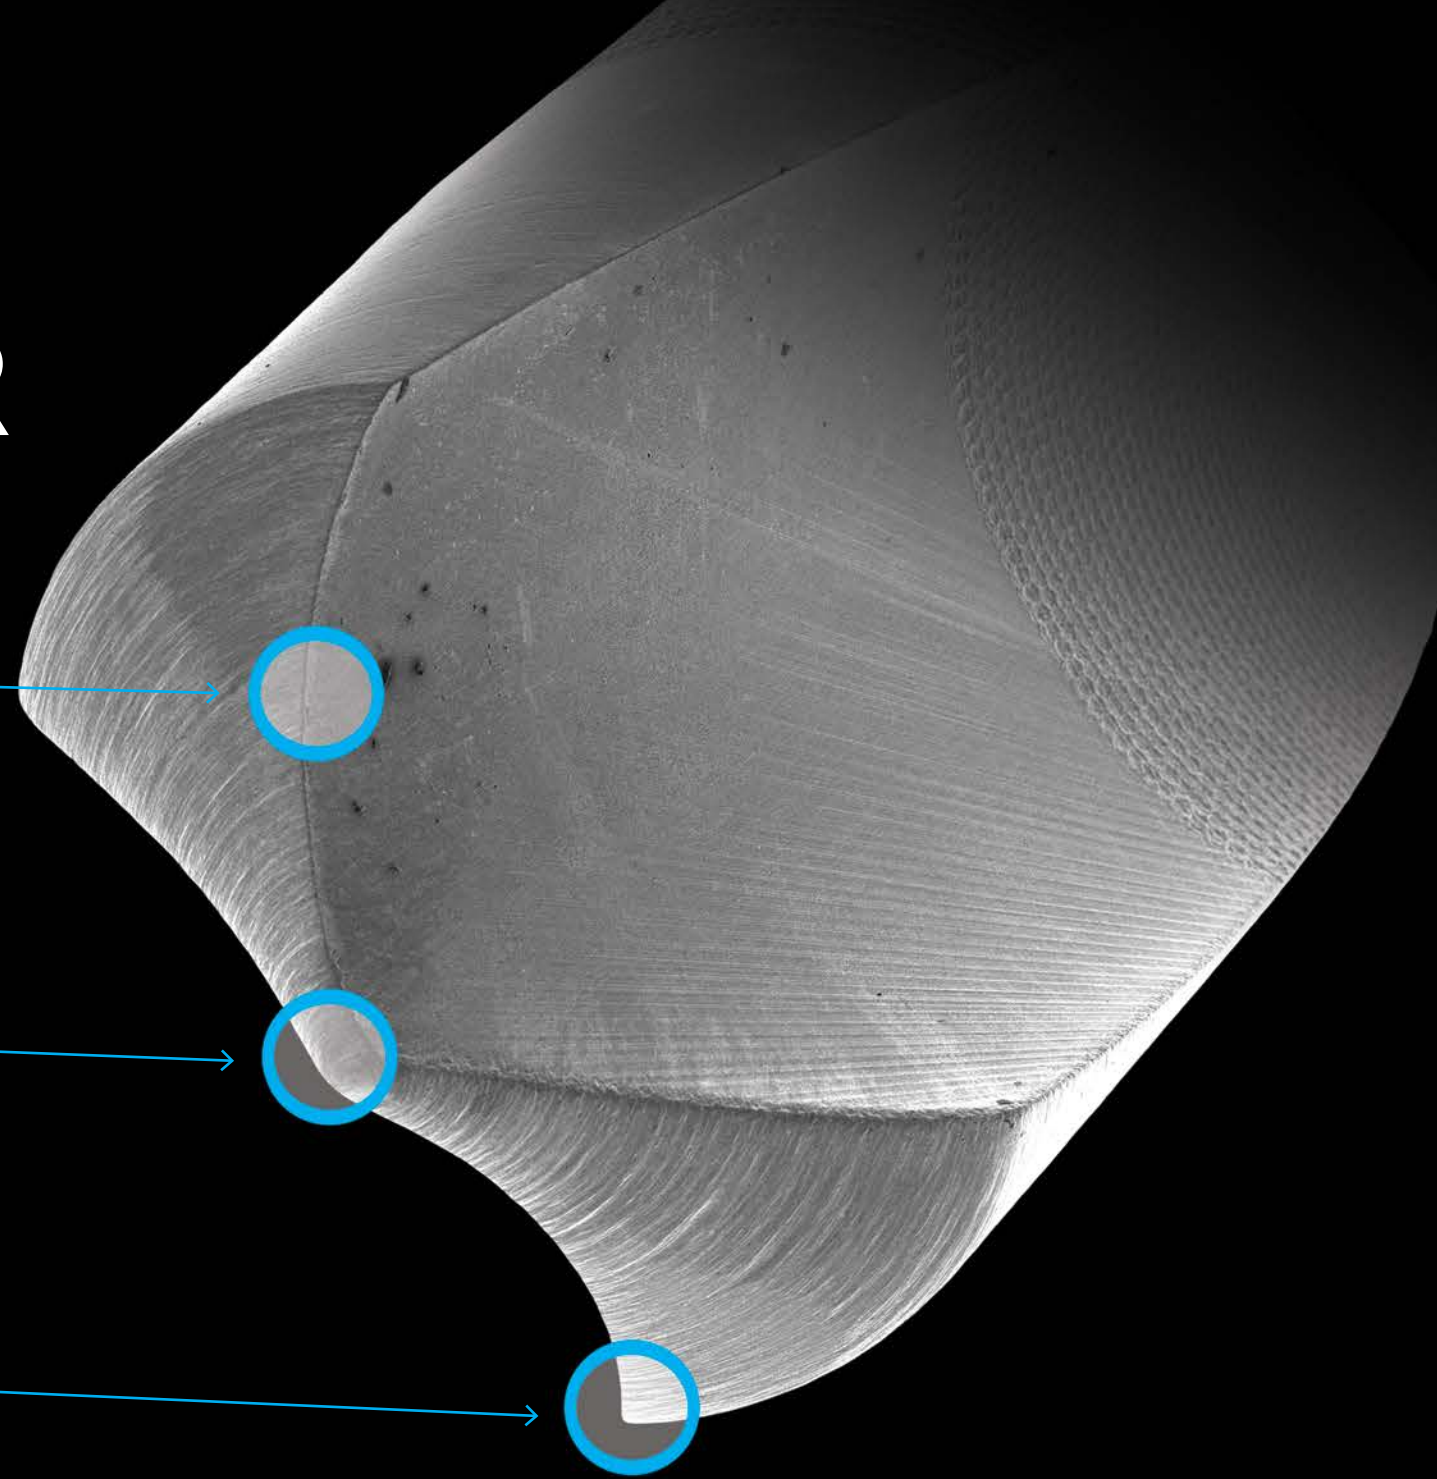

## Inspection for Wear and Damage

Before each use, visually inspect all devices and trays/kits for completeness, damage and/or excessive wear (e.g. corrosion or rust build-up on the instrument surface, structural wear or damage, grommet presence or damage partial or complete fracture. If damage or wear is noted that may compromise the function of the instrument or tray, **DO NOT USE**. Contact your Zimmer Biomet representative for replacement.

Refer to Instructions for Use (IFU) for Zimmer Instrument Kits, Drills and Tools available at <https://labeling.zimmerbiomet.com> for complete Cleaning and Sterilization Information.

