

# Puros<sup>®</sup> Ci Particulate Allograft



## OPTIMAL BLEND OF SCAFFOLD AND OSTEOINDUCTIVE POTENTIAL

### 1 Ideal Blend<sup>1</sup>

- Combination of mineralized and demineralized allograft bone (DBM)
- Only DBM with verified osteoinductive (OI) potential<sup>\*</sup> is released for processing
- Mineralized component acts as a scaffold; Mineralized particles include both cancellous and cortical bone chips

### 2 Best In Class Processing<sup>1</sup>

- Proprietary Tutoplast<sup>™</sup> processing preserves the native collagen matrix of the mineralized particles
- Proprietary Cancellle SP<sup>®</sup> processing preserves OI potential

### 3 Trusted Source<sup>1</sup>

- Safety and reliability you expect from the Puros Brand
- Single donor source for mineralized and demineralized particles
- Terminally sterilized to SAL 10<sup>-6</sup>

### 4 Convenient Handling

- Quick hydration
- Room temperature storage<sup>2</sup>

<sup>1</sup>DBM is evaluated for bone formation utilizing an in-vivo athymic rat model. Findings from an animal model are not necessarily predictive of human clinical results.



**Puros® Ci** is a unique combination of cancellous, cortical and demineralized cortical bone designed for filling bone voids.


### TUTOPLAST PROCESS<sup>1</sup>

The **Tutoplast Process** is a proprietary process that preserves biomechanical/biochemical integrity and native tissue structure. Over the past **20 years**:

1. Approximately **6 million implants** have gone through the Tutoplast Process globally
2. More than **5.5 million patient procedures** have been performed using implants processed through the Tutoplast Process globally
3. **Zero** confirmed incidence of implant-associated infection

### CANCELLE SP PROCESS<sup>1</sup>

The **Cancelle SP Process** is a proprietary process that sterilizes DBM while simultaneously allowing it to maintain its OI potential.

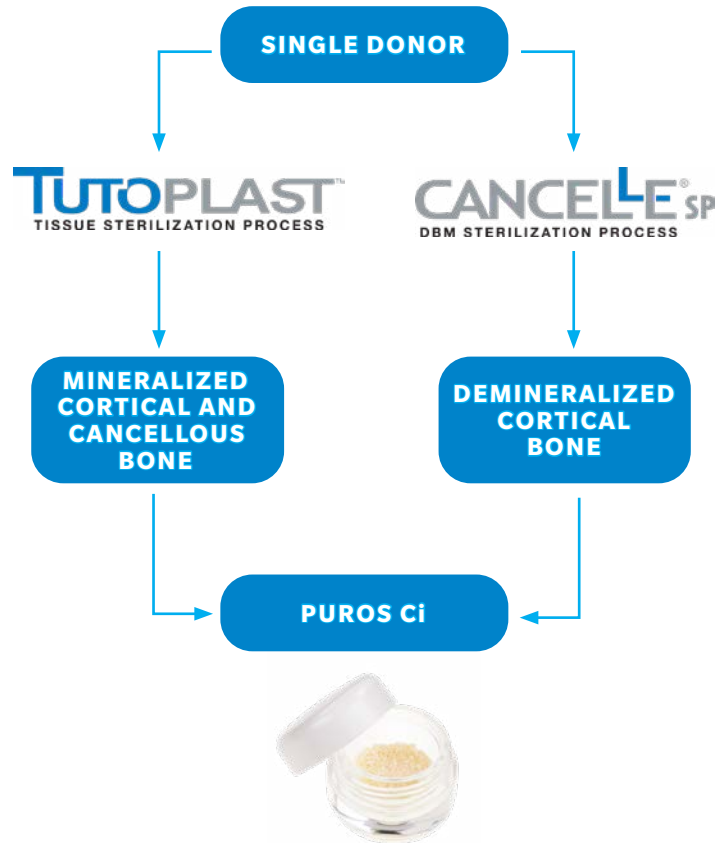

### ORDERING INFORMATION:

Description	Item No.
Puros Ci Particulate Allograft, 0.5 cc, .25 – 1 mm	69800
Puros Ci Particulate Allograft, 1 cc, .25 – 1 mm	69801
Puros Ci Particulate Allograft, 2 cc, .25 – 1 mm	69802
Puros Ci Particulate Allograft, 0.5 cc, 1 – 2 mm	69803
Puros Ci Particulate Allograft, 1 cc, 1 – 2 mm	69804
Puros Ci Particulate Allograft, 2 cc, 1 – 2 mm	69805

<sup>1</sup>Data on file with RTI Surgical, Inc.

<sup>2</sup>Refer to product label for specific storage parameters.



Contact us at 1-800-342-5454 or visit [zimmerbiometdental.com](http://zimmerbiometdental.com)

Zimmer Biomet Dental  
Global Headquarters  
4555 Riverside Drive  
Palm Beach Gardens, FL 33410  
Phone: +1-561-776-6700  
Fax: +1-561-776-1272

Unless otherwise indicated, as referenced herein, all trademarks are the property of Zimmer Biomet; and all products are manufactured by one or more of the dental subsidiaries of Zimmer Biomet Holdings, Inc. and marketed and distributed by Zimmer Biomet Dental and its authorized marketing partners. Cancelle SP is a U.S. registered trademark of RTI Surgical, Inc. Puros is manufactured by RTI Surgical, Inc. Tutoplast is a registered trademark of Tutogen Medical GmbH. For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited. This material may not be copied or reprinted without the express written consent of Zimmer Biomet Dental. ZB1025 REV A 03/20 ©2020 Zimmer Biomet. All rights reserved.

